

Assessing Clinical Response in Multiple Myeloma (MM) Patients Treated With Monoclonal Antibodies (Mabs): Validation of a Daratumumab IFE Reflex Assay (DIRA) to Distinguish Malignant M-Protein From Therapeutic Antibody

Christopher McCudden,^{1,*} Amy Axel,² Dominique Slaets,³ Sandy Frans,⁴ Jaime Bald,² Jordan Schecter,⁵ Tahamtan Ahmadi,² Torben Plesner,⁶ Kate Sasser²

¹Dept. of Pathology & Laboratory Medicine, The Ottawa Hospital/University of Ottawa, Ottawa ON, Canada; ²Janssen Research & Development, LLC, Spring House, PA, USA; ³BARC, a division of CERBA European Lab, Ghent, Belgium; ⁴Janssen Research & Development, LLC, Beerse, Belgium; ⁵Janssen Research & Development, LLC, Raritan, NJ, USA; ⁶Vejle Hospital and University of Southern Denmark, Vejle, Denmark.

*Presenting author.

INTRODUCTION

In multiple myeloma (MM), malignant plasma cells secrete high levels of monoclonal immunoglobulin protein (M-protein) that are detectable by serum protein electrophoresis (SPEP) or immunofixation electrophoresis (IFE; **Figure 1**)

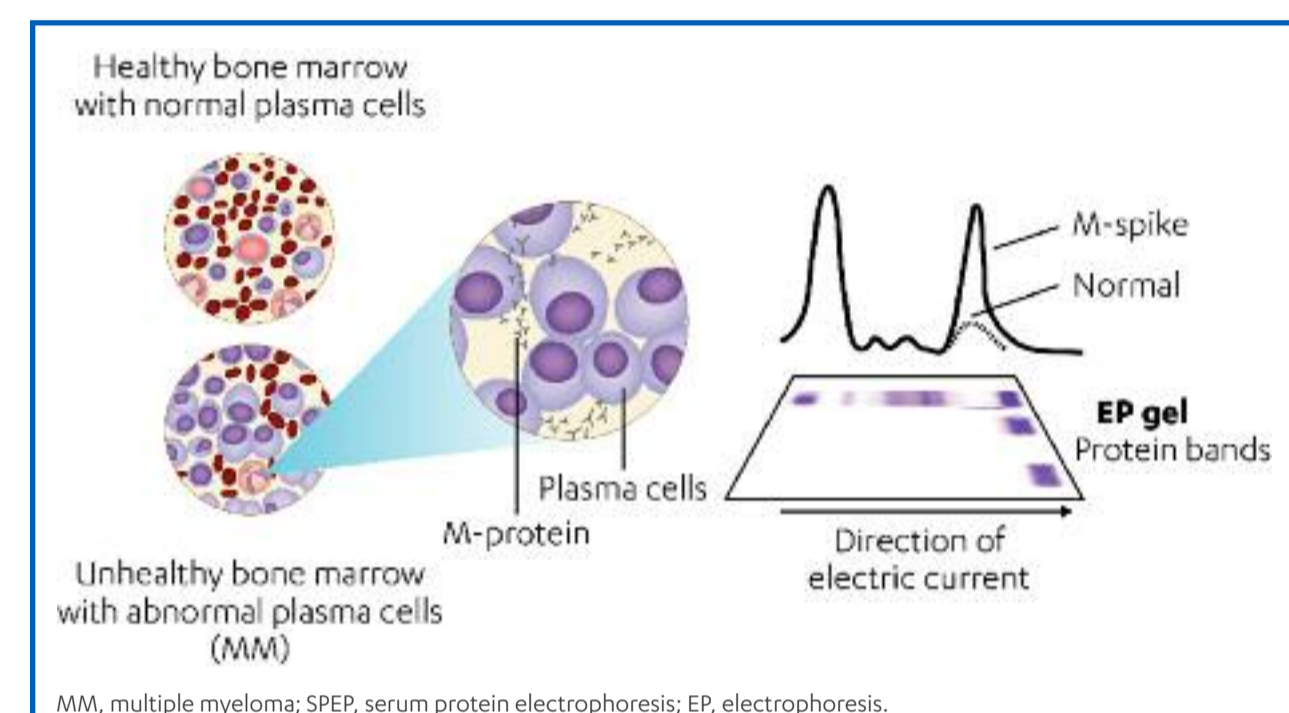


Figure 1. MM cells secrete high levels of M-protein detectable by SPEP.

International Myeloma Working Group (IMWG) criteria require that patients' serum samples are negative for M-protein by SPEP/IFE in order to claim complete response (CR) or stringent CR (sCR; **Figure 2**)²

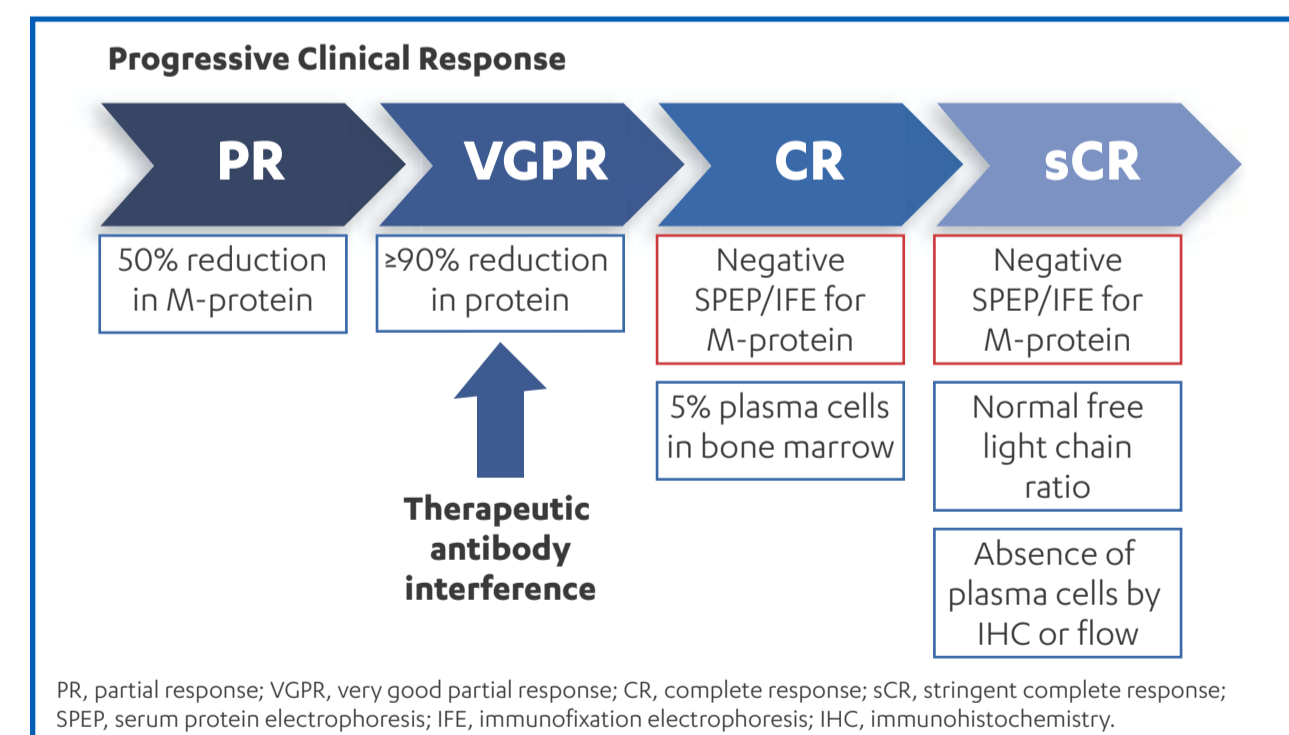


Figure 2. Therapeutic antibodies may interfere with the ability to confirm clinical outcomes deeper than very good partial responses.

Monoclonal antibodies have shown therapeutic efficacy in a number of malignancies, but they may interfere with interpretation of IFE data^{3,4}

Daratumumab is a CD38 IgG1κ monoclonal antibody (mAb) in clinical development for the treatment of MM⁵

Daratumumab has demonstrated clinical responses that deepen over time, necessitating evaluation of CR/sCR by SPEP/IFE⁷

Approximately 50% of patients with MM produce an IgGκ M-protein. In a subset of patients, either daratumumab or the daratumumab-anti-idiotype complex may co-migrate with endogenous M-protein⁸

Steady-state concentrations of daratumumab (dosed at 16 mg/kg weekly, bi-monthly, and then monthly) are readily detectable on most SPEP and IFE assays⁸

OBJECTIVE

Validate and implement a daratumumab interference reflex assay (DIRA) that distinguishes M-protein from daratumumab, as assessed by IFE, in order to determine if additional testing to assess CR/sCR is warranted (ie, bone marrow examination)

Schematics of idealized gels for DIRA-negative and DIRA-positive samples are shown in **Figure 3**

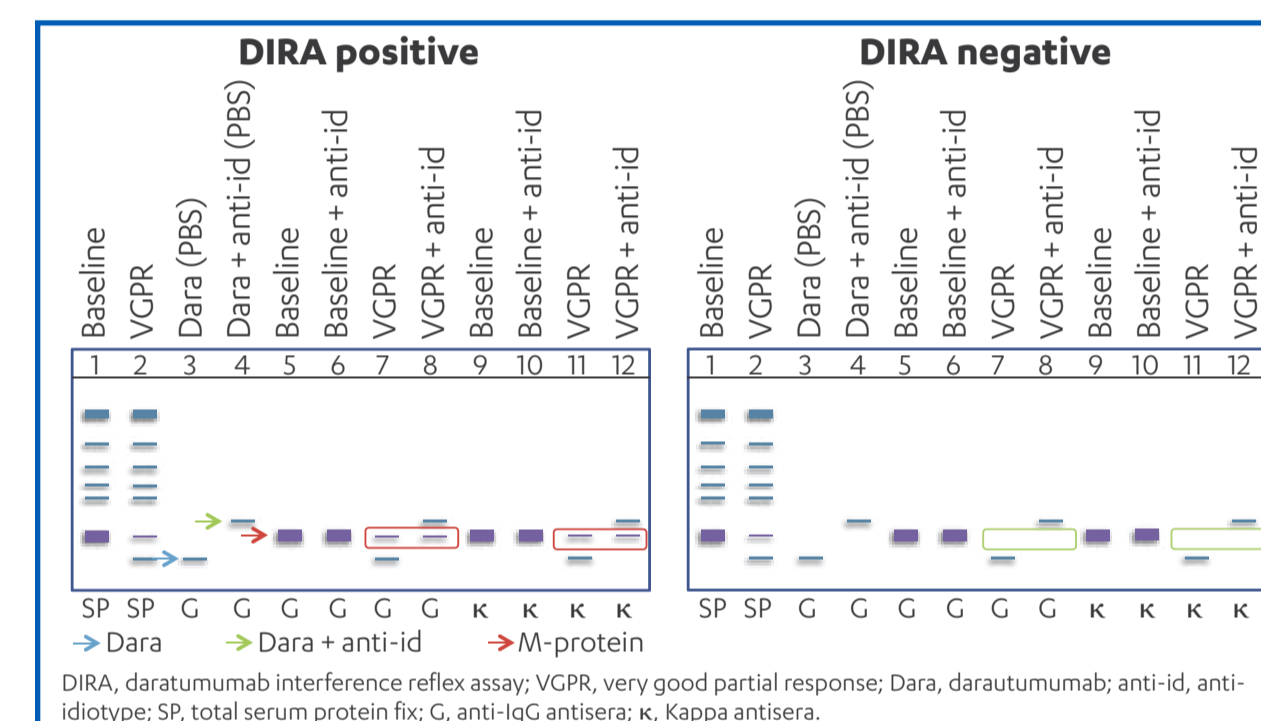


Figure 3. Schematic Presentation of DIRA-positive and DIRA-negative daratumumab-treated Patient Samples

METHODS

Patient Samples

Human serum samples from patients with MM (n = 51) were acquired from a commercial source or from patients treated with daratumumab in clinical trials (n = 33)

IFE

Serum IFE assays were performed using Maxikit Hydragel 9IF Kits (Sebia Electrophoresis, Norcross, GA) according to the manufacturer's specifications

Antisera against immunoglobulins gamma (IgG), alpha, and mu heavy chains and free and bound kappa (κ) and lambda light chains were used to characterize the monoclonal protein present in each sample

DIRA

Serum samples for baseline and daratumumab-treated patients were incubated with or without an anti-idiotype mAb (mouse-anti-HuMax-CD38; clone 5-3-9-4) at room temperature for 15 minutes and analyzed by IFE with IgG and Igκ antisera

Specificity

To demonstrate that the anti-idiotype antibody binds and shifts daratumumab without affecting detection and migration of endogenous M-protein, commercially available serum samples from patients with MM (n = 51) were spiked with daratumumab, anti-idiotype, or daratumumab + anti-idiotype (500 and 1,000 μg/mL; 1:1 ratio) IgG and Igκ, and were then analyzed by IFE to assess changes in migration of M-protein

Lower Limit of Detection

Lower limit of detection (LOD) was determined by evaluating daratumumab ± anti-idiotype over a clinically relevant dynamic range to determine the lowest concentration detected by ≥1 parameter (daratumumab IgG, daratumumab + anti-idiotype complex IgG, daratumumab Igκ, daratumumab + anti-idiotype Igκ for IFE; daratumumab or daratumumab + anti-idiotype by SPEP)

Reproducibility

Three independent runs of 10 samples from daratumumab-treated patients, who had achieved PR or better and M-protein ≤5 g/dL, were performed using DIRA, and the results (DIRA-positive or DIRA-negative) were assessed for reproducibility

Concordance

Two independent reviewers interpreted all results

RESULTS

The DIRA template utilized daratumumab ± anti-idiotype as controls for migration of the therapeutic antibody and the daratumumab-anti-idiotype shifted couples. Baseline and post-treatment serum ± anti-idiotype were compared to determine whether M-protein remained after shifting daratumumab. DIRA-positive results showed M-protein, whereas DIRA-negative results showed only a shift in daratumumab but no remaining M-protein (lanes 8, 12; **Figure 4**)

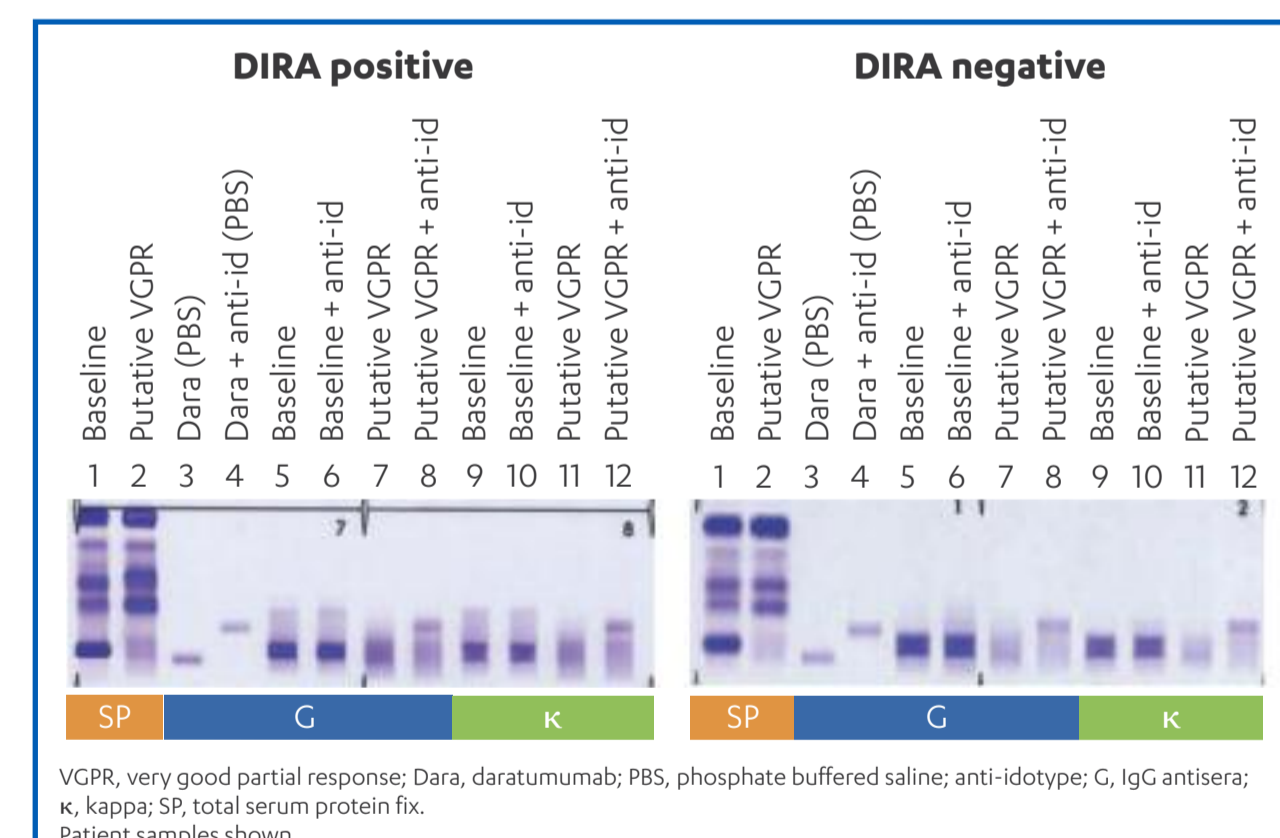


Figure 4. Example of DIRA-positive and DIRA-negative daratumumab-treated patient samples.

Specificity

Daratumumab was shifted by the anti-idiotype at all concentrations in 51 of 51 samples

In 47 of 51 samples (92%), no alteration in banding pattern occurred when either concentration of anti-idiotype (500 and 1,000 μg/mL) was introduced, indicating that no nonspecific binding was observed

In 4 of 51 samples (8%), a faint band appeared with the addition of anti-idiotype at both concentrations with IgG antisera

A representative gel, with no change in banding pattern, is shown in **Figure 5A**; the faint band is apparent in **Figure 5B**, lane 8

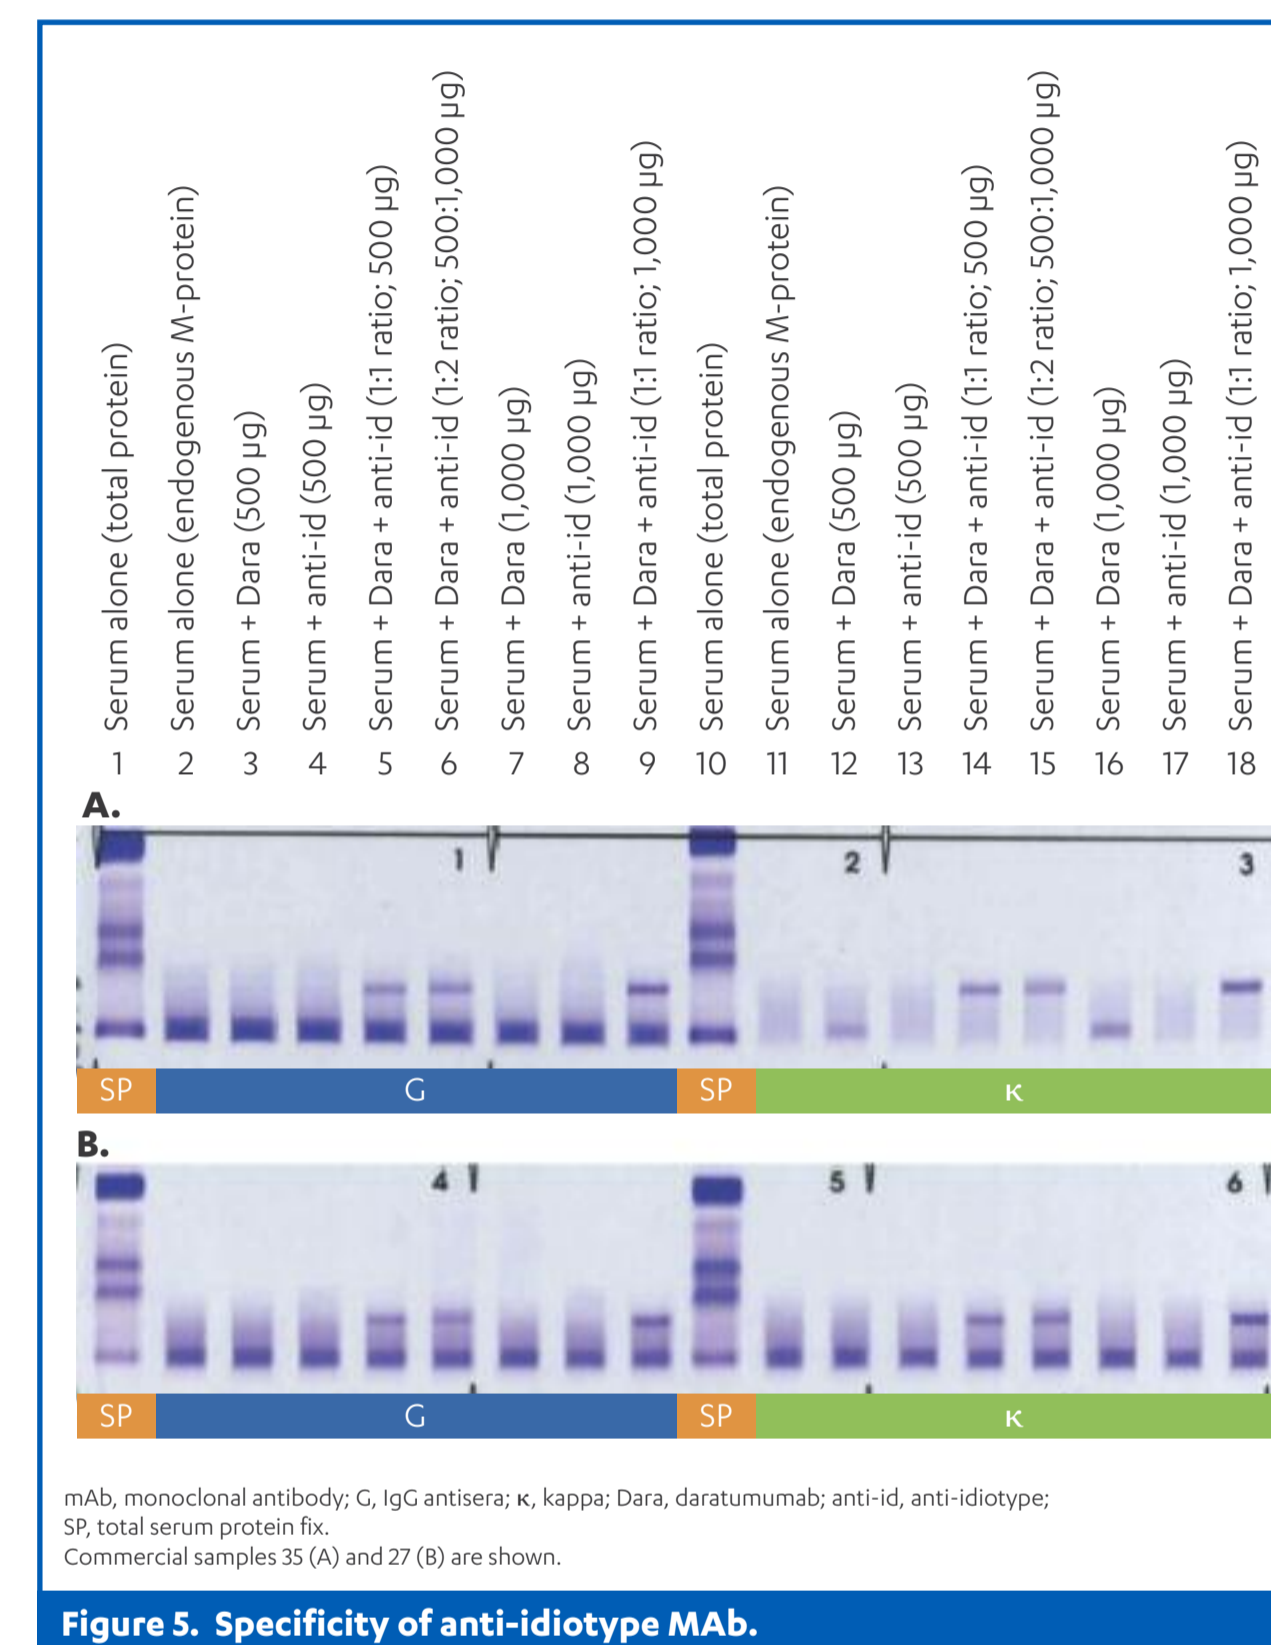


Figure 5. Specificity of anti-idiotype MAb.

Lower Limit of Detection

In MM serum samples, daratumumab could be detected by IFE at 100 μg/mL in 9 of 10 samples by ≥1 parameter and at 200 μg/mL in 10 of 10 samples

In the same samples analyzed by SPEP, either daratumumab and/or daratumumab plus anti-idiotype complex could be identified at 100 μg/mL in 3 of 10 samples and by 200 μg/mL in 10 of 10 samples

Examining the totality of all parameters (daratumumab [IgG], daratumumab + anti-id [IgG], daratumumab [Igκ], daratumumab + anti-id [Igκ] for all 10 samples), the lowest detectable concentration of daratumumab was 100 μg/mL in 26 of 40 samples, 200 μg/mL in 10 of 40 samples, 250 μg/mL in 1 of 40 samples, 500 μg/mL in 1 of 40, and comigrating (undetectable) in 2 of 40 samples

DIRA Reproducibility and Concordance

In 10 of 10 (100%) daratumumab-treated patient samples, results were consistent across all 3 independent runs

Results from all repetitions from a representative patient sample are shown in **Figure 6**

There was 100% concordance between the evaluations of 2 independent reviewers

Reviewer evaluations were standardized using a brief form with set assessment criteria; those criteria and the reviewers' responses assessing the sample shown in **Figure 6** are tallied in **Table 1**

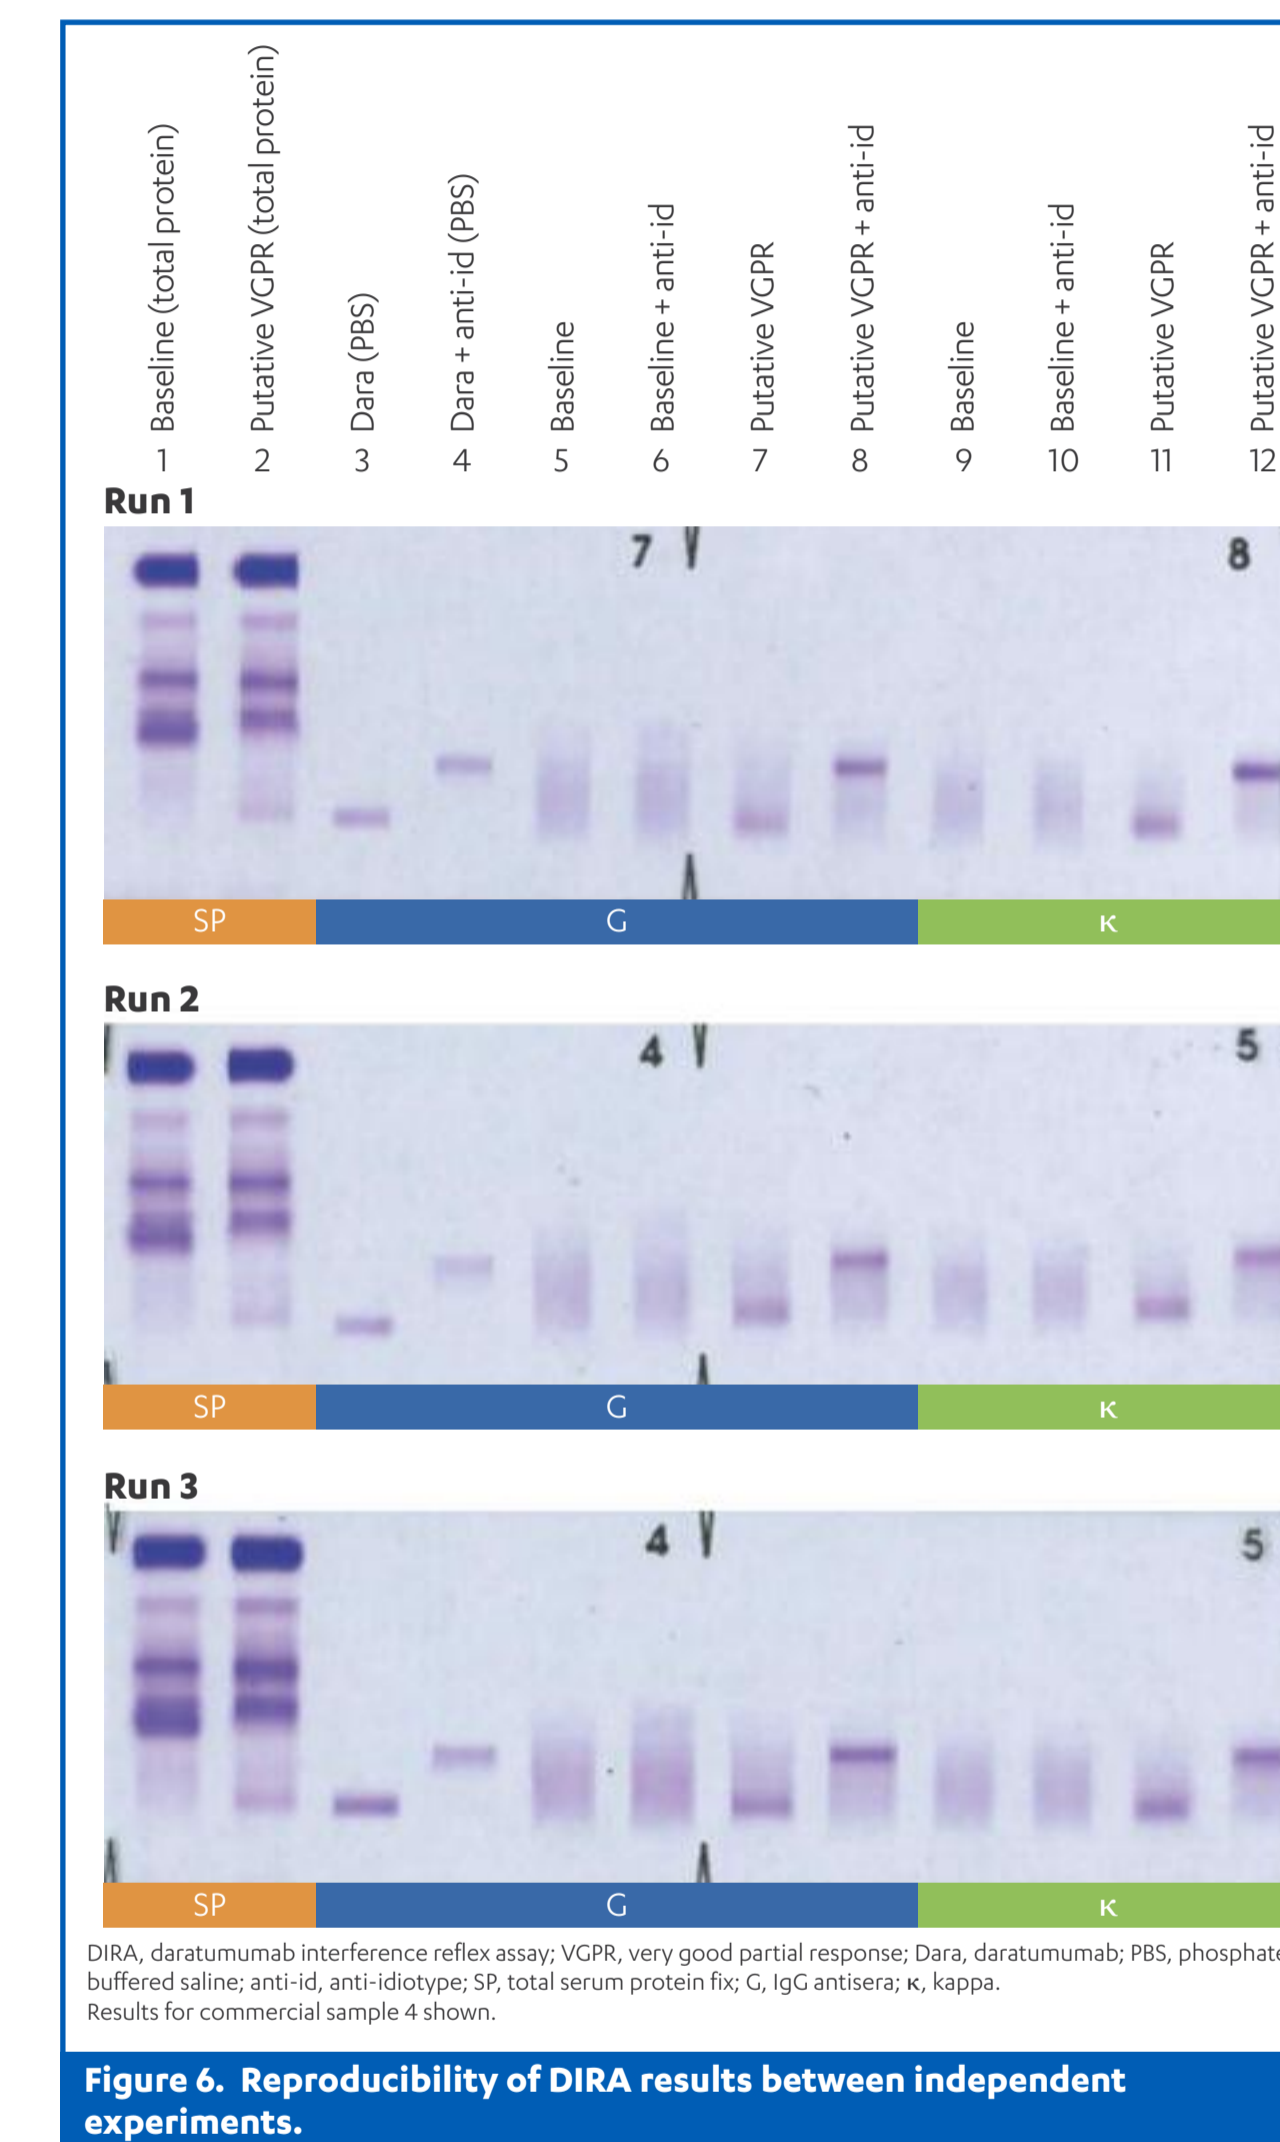


Figure 6. Reproducibility of DIRA results between independent experiments.

Identification of Clinical Responses

DIRA differentiated daratumumab-treated patient samples containing residual M-protein (DIRA-positive) from those containing no M-protein (DIRA-negative)

33 samples from daratumumab-treated patients from a number of different studies were assessed for clinical response using DIRA

13 patients (39%) were DIRA-negative, 10 of whom were confirmed as having achieved CR based on bone marrow and FLC

20 (61%) were DIRA-positive and will continue to be monitored

ACKNOWLEDGMENTS

This study was supported by Janssen Research & Development, LLC. Editorial support was provided by Erica Chevalier-Larsen, PhD, of MedErgy, and was funded by Janssen Global Services, LLC.

Table 1. Concordance of Reviewer Assessments Between Experiments

Reviewer 1	Lane	Run 1	Run 2	Run 3
Migration of Dara + anti-id in control?	4 vs 3	Y	Y	Y
Migration of endogenous M-protein at baseline?	6 and 10	N	N	N
Migration of Dara in VGPR due to the disappearance of Dara (DD) or the appearance of Dara + anti-id complex (AC)?	8 vs 7 and 12 vs 11	Y DD + AC	Y DD + AC	Y DD + AC
Presence of M-protein after migration of Dara?	8 and 12	N	N	N
M-protein (M) or Dara (D)?		D	D	D
Conclusion		Negative	Negative	Negative
Reviewer 2	Lane	Run 1	Run 2	Run 3
Migration of Dara + anti-id in control?	4 vs 3	Y	Y	Y
Migration of endogenous M-protein at baseline?	6 and 10	N	N	N
Migration of Dara in VGPR due to the disappearance of Dara (DD) or the appearance of Dara + anti-id complex (AC)?	8 vs 7 and 12 vs 11	Y DD + AC	Y DD + AC	Y DD + AC
Presence of M-protein after migration of Dara?	8 and 12	N	N	N
M-protein (M) or Dara (D)?		D	D	D
Conclusion		Negative	Negative	Negative

CONCLUSIONS

DIRA is a specific, reproducible method to confirm the interference of daratumumab on serum IFE at 100 to 200 μg/mL

DIRA-negative status warrants additional testing to confirm CR/sCR

IMWG response criteria may require modification as mAbs receive approval for the treatment of MM

REFERENCES

- Zent CS, et al. *Blood*. 1998;91(9):3518-3523.
- Rajkumar SV, et al. *Blood*. 2011;117(18):4691-4695.
- McCudden CR, et al. *Clin Chem*. 2010;56(12):1897-1899.
- Genzen JR, et al. *Br J Haematol*. 2011;155(1):123-125.
- de Weers M, et al. *J Immunol*. 2011;186(3):1840-1848.
- Lokhorst HM, et al. *J Clin Oncol*. 2014;32(15 suppl): Abstract 8513.
- Plesner T, et al. *Blood*. 2014;124(21):84.
- Axel AE, et al. Presented at: Annual Meeting of the American Association for Cancer Research; April 5-9, 2014; San Diego, CA. Abstract 2563.



An electronic version of the poster can be viewed by scanning the QR code. The QR code is intended to provide scientific information for individual reference. The PDF should not be altered or reproduced in any way.

Copies of this poster obtained through Quick Response (QR) Code are for personal use only and may not be reproduced without permission from ASCO® and the author of this poster.

INTRODUCTION

- ◆ In multiple myeloma (MM), malignant plasma cells secrete high levels of monoclonal immunoglobulin protein (M-protein) that are detectable by serum protein electrophoresis (SPEP) or immunofixation electrophoresis¹ (IFE; **Figure 1**)

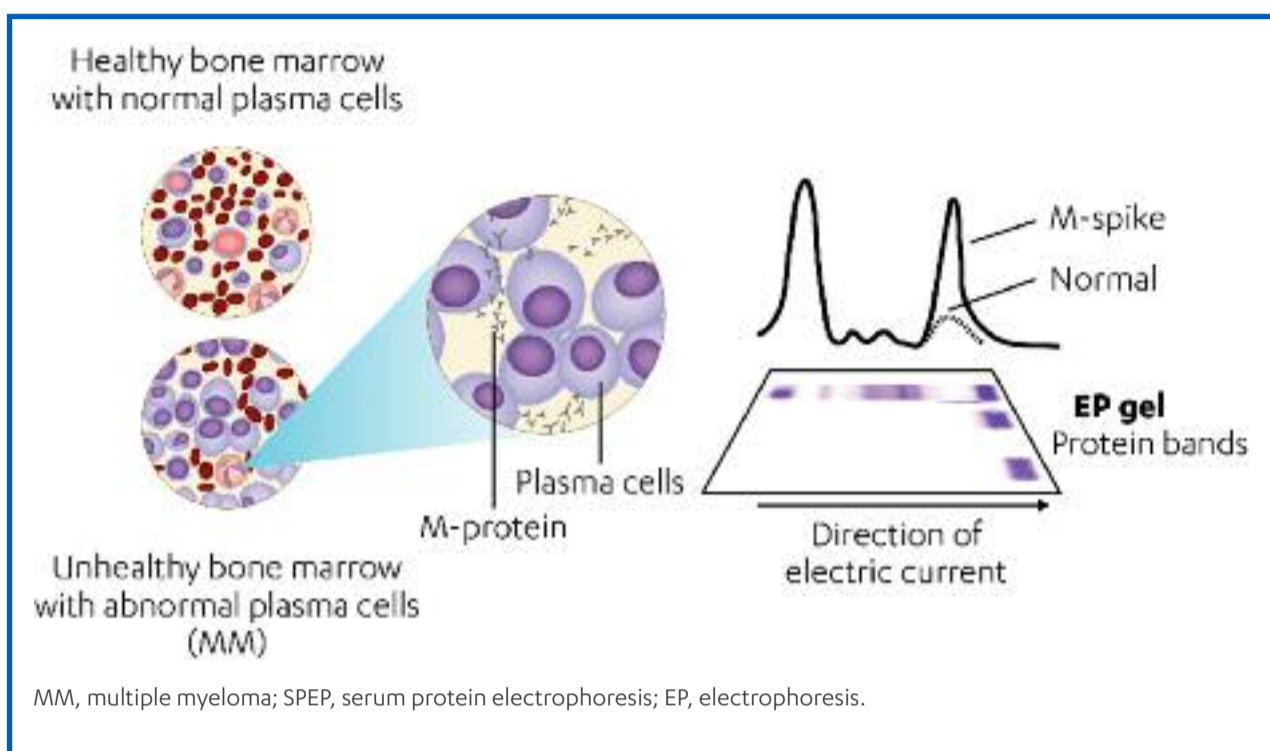


Figure 1. MM cells secrete high levels of M-protein detectable by SPEP.

- ◆ International Myeloma Working Group (IMWG) criteria require that patients' serum samples are negative for M-protein by SPEP/IFE in order to claim complete response (CR) or stringent CR (sCR; **Figure 2**)²

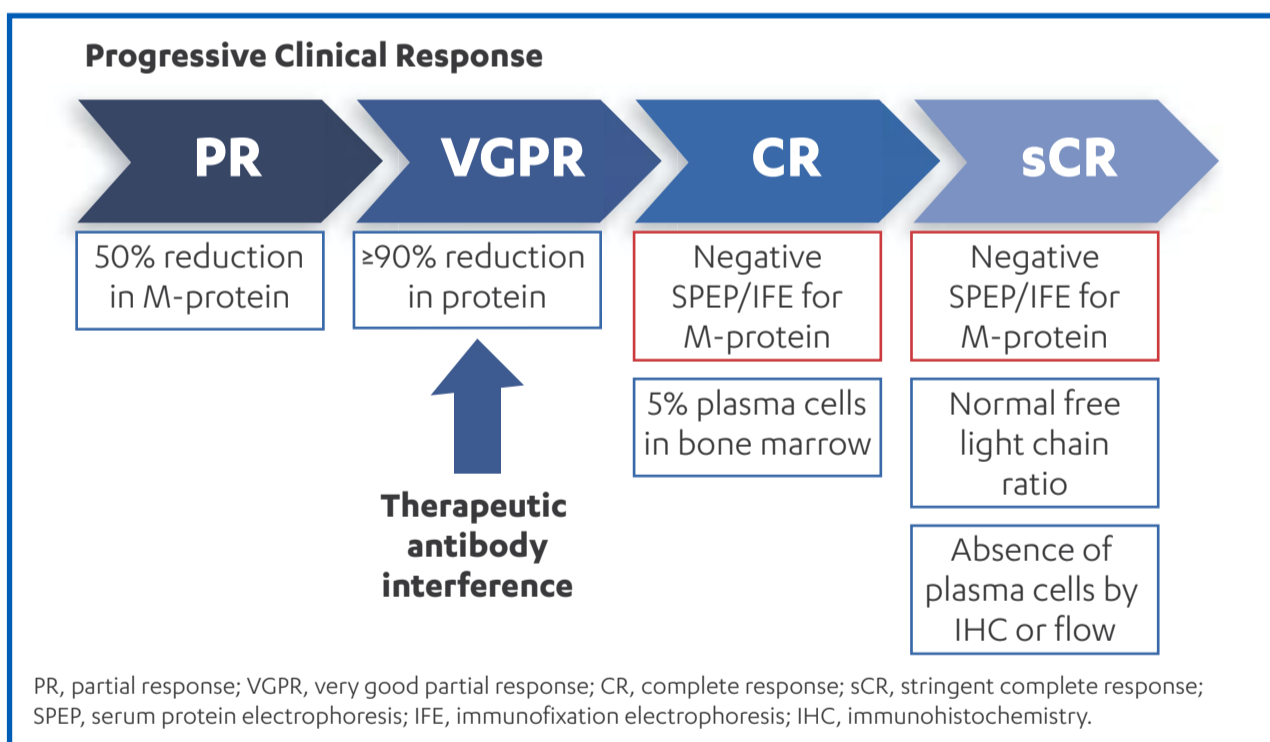


Figure 2. Therapeutic antibodies may interfere with the ability to confirm clinical outcomes deeper than very good partial responses.

- ◆ Monoclonal antibodies have shown therapeutic efficacy in a number of malignancies, but they may interfere with interpretation of IFE data^{3,4}
- ◆ Daratumumab is a CD38 IgG1κ monoclonal antibody (mAb) in clinical development for the treatment of MM⁵
- ◆ Daratumumab has demonstrated clinical responses that deepen over time, necessitating evaluation of CR/sCR by SPEP/IFE^{6,7}
 - Approximately 50% of patients with MM produce an IgGκ M-protein. In a subset of patients, either daratumumab or the daratumumab–anti-idiotypic complex may co-migrate with endogenous M-protein⁸

- Steady-state concentrations of daratumumab (dosed at 16 mg/kg weekly, bi-monthly, and then monthly) are readily detectable on most SPEP and IFE assays⁸

OBJECTIVE

- Validate and implement a daratumumab interference reflex assay (DIRA) that distinguishes M-protein from daratumumab, as assessed by IFE, in order to determine if additional testing to assess CR/sCR is warranted (ie, bone marrow examination)
 - Schematics of idealized gels for DIRA-negative and DIRA-positive samples are shown in **Figure 3**

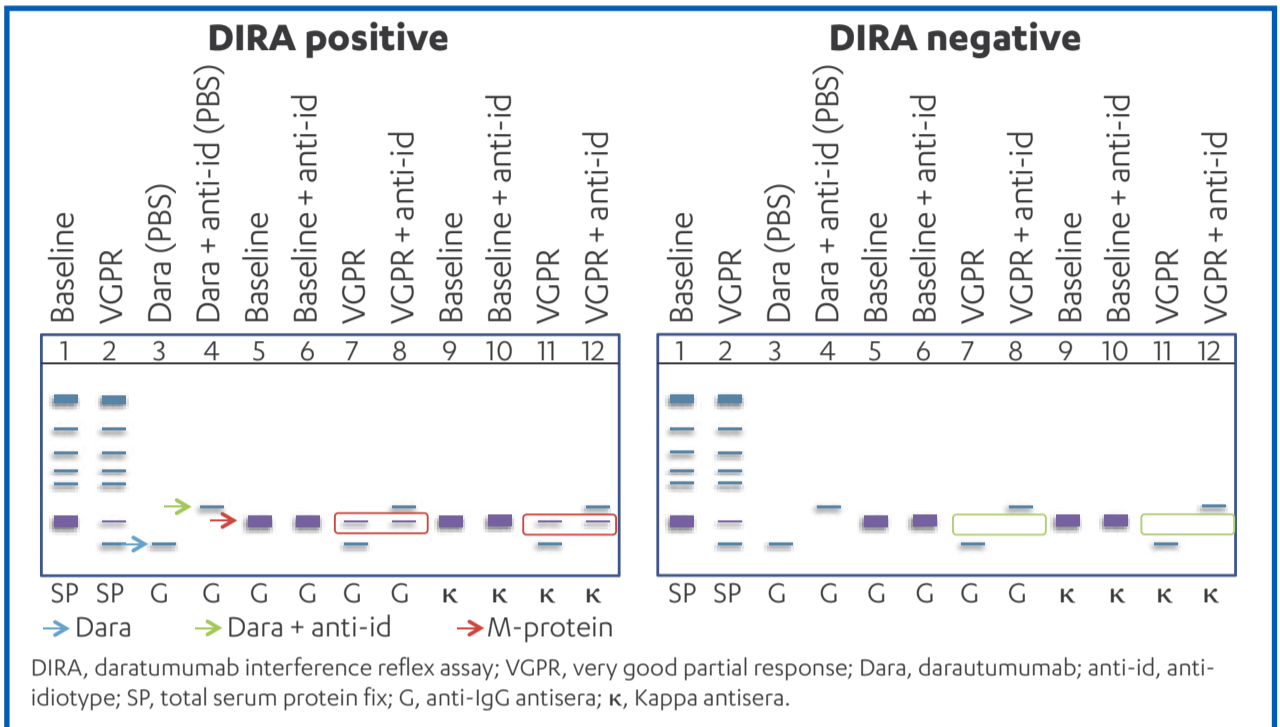


Figure 3. Schematic Presentation of DIRA-positive and DIRA-negative daratumumab-treated Patient Samples

METHODS

Patient Samples

- Human serum samples from patients with MM (n = 51) were acquired from a commercial source or from patients treated with daratumumab in clinical trials (n = 33)

IFE

- Serum IFE assays were performed using Maxikit Hydragel 9IF Kits (Sebia Electrophoresis, Norcross, GA) according to the manufacturer's specifications
- Antisera against immunoglobulins gamma (IgG), alpha, and mu heavy chains and free and bound kappa (κ) and lambda light chains were used to characterize the monoclonal protein present in each sample

DIRA

- Serum samples for baseline and daratumumab-treated patients were incubated with or without an anti-idiotype mAb (mouse-anti-HuMax-CD38; clone 5-3-9-4) at room temperature for 15 minutes and analyzed by IFE with IgG and Igκ antisera

Specificity

- To demonstrate that the anti-idiotype antibody binds and shifts daratumumab without affecting detection and migration of endogenous M-protein, commercially available serum samples from patients with MM (n = 51) were spiked with daratumumab, anti-idiotype, or daratumumab + anti-idiotype (500 and 1,000 μg/mL; 1:1 ratio) IgG and Igκ, and were then analyzed by IFE to assess changes in migration of M-protein

Lower Limit of Detection

- ◆ Lower limit of detection (LOD) was determined by evaluating daratumumab ± anti-idiotype over a clinically relevant dynamic range to determine the lowest concentration detected by ≥1 parameter (daratumumab IgG, daratumumab + anti-idiotype complex IgG, daratumumab Igκ, daratumumab + anti-idiotype Igκ for IFE; daratumumab or daratumumab + anti-idiotype by SPEP)

Reproducibility

- ◆ Three independent runs of 10 samples from daratumumab-treated patients, who had achieved PR or better and M-protein ≤5 g/dL, were performed using DIRA, and the results (DIRA-positive or DIRA-negative) were assessed for reproducibility

Concordance

- ◆ Two independent reviewers interpreted all results

RESULTS

- ◆ The DIRA template utilized daratumumab ± anti-idiotype as controls for migration of the therapeutic antibody and the daratumumab–anti-idiotype shifted couples. Baseline and post-treatment serum ± anti-idiotype were compared to determine whether M-protein remained after shifting daratumumab. DIRA-positive results showed M-protein, whereas DIRA-negative results showed only a shift in daratumumab but no remaining M-protein (lanes 8, 12; **Figure 4**)


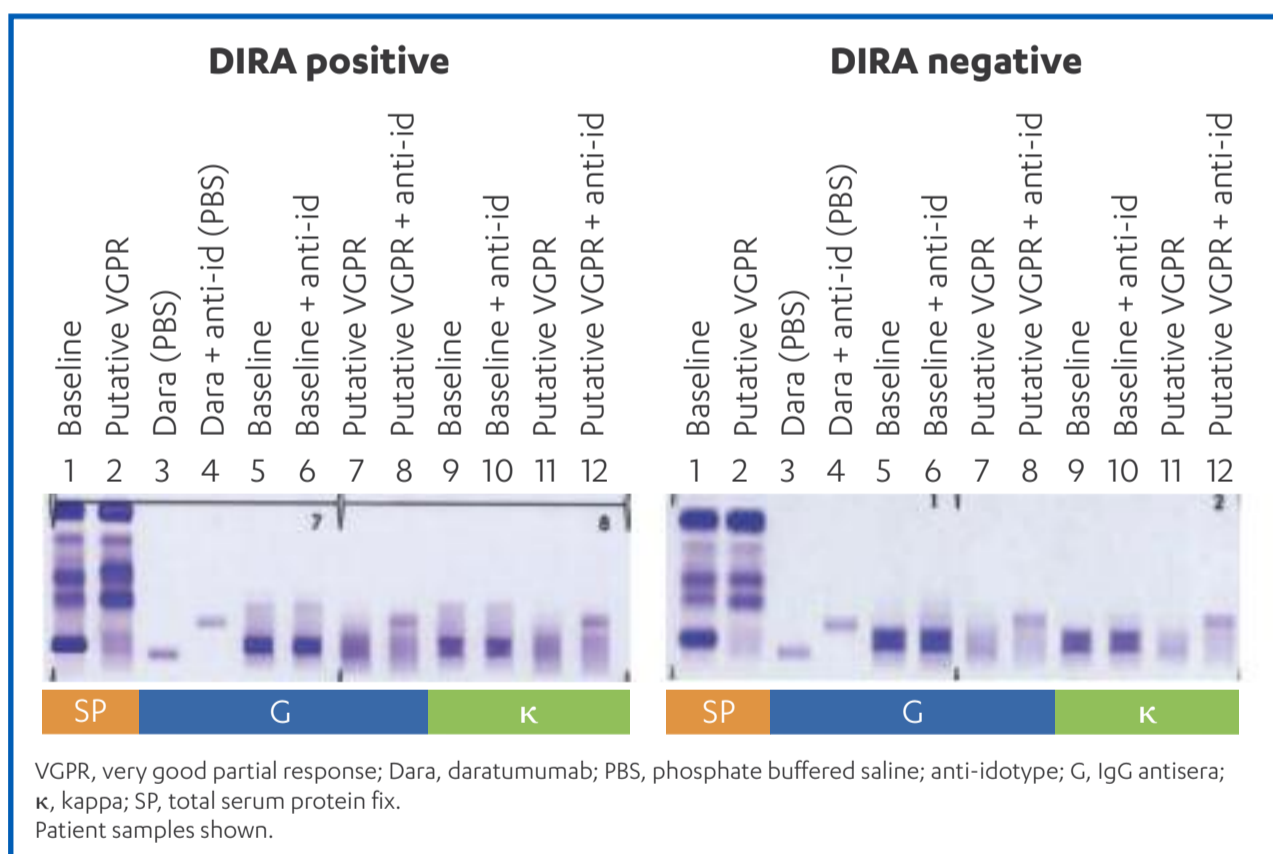


Figure 4. Example of DIRA-positive and DIRA-negative daratumumab-treated patient samples.

Specificity

- ◆ Daratumumab was shifted by the anti-idiotype at all concentrations in 51 of 51 samples
- ◆ In 47 of 51 samples (92%), no alteration in banding pattern occurred when either concentration of anti-idiotype (500 and 1,000 μg/mL) was introduced, indicating that no nonspecific binding was observed
- ◆ In 4 of 51 samples (8%), a faint band appeared with the addition of anti-idiotype at both concentrations with IgG antisera
 - A representative gel, with no change in banding pattern, is shown in **Figure 5A**; the faint band is apparent in **Figure 5B**, lane 8

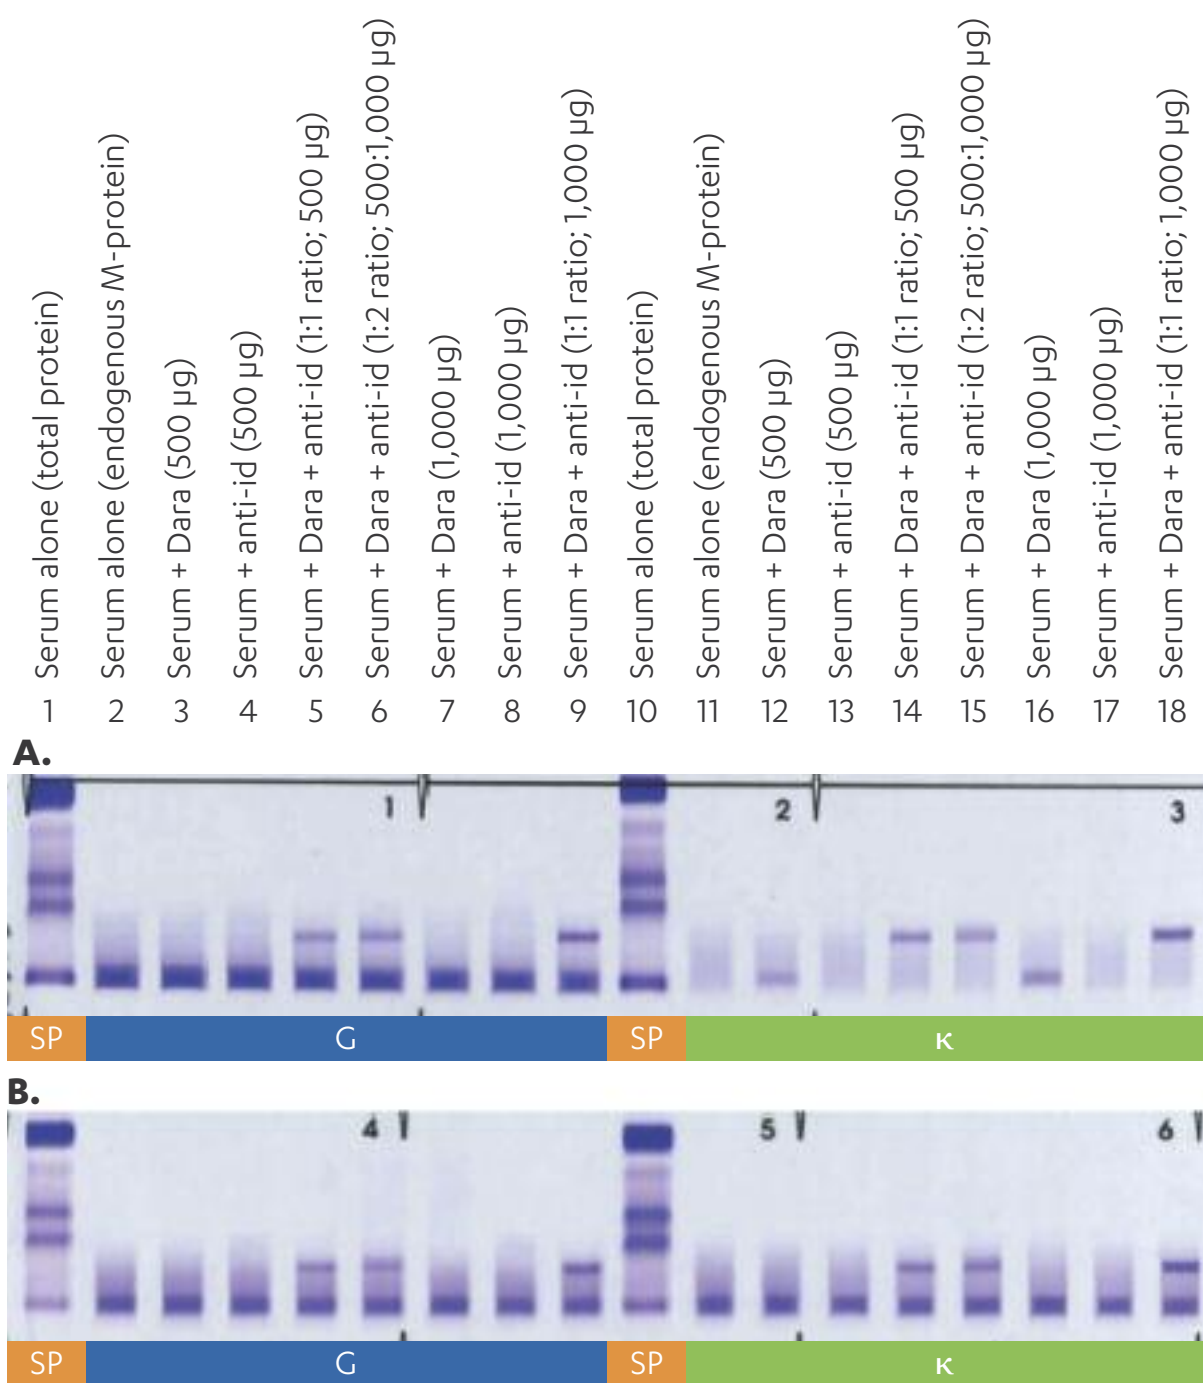

mAb, monoclonal antibody; G, IgG antisera; κ, kappa; Dara, daratumumab; anti-id, anti-idiotype; SP, total serum protein fix. Commercial samples 35 (A) and 27 (B) are shown.


Figure 5. Specificity of anti-idiotype MAb.

Lower Limit of Detection

- ◆ In MM serum samples, daratumumab could be detected by IFE at 100 µg/mL in 9 of 10 samples by ≥1 parameter and at 200 µg/mL in 10 of 10 samples
 - In the same samples analyzed by SPEP, either daratumumab and/or daratumumab plus anti-idiotype complex could be identified at 100 µg/mL in 3 of 10 samples and by 200 µg/mL in 10 of 10 samples
- ◆ Examining the totality of all parameters (daratumumab [IgG], daratumumab + anti-id [IgG], daratumumab [Igκ], and dara + anti-id [Igκ] for all 10 samples), the lowest detectable concentration of daratumumab was 100 µg/mL in 26 of 40 samples, 200 µg/mL in 10 of 40 samples, 250 µg/mL in 1 of 40 samples, 500 µg/mL in 1 of 40, and comigrating (undetectable) in 2 of 40 samples

DIRA Reproducibility and Concordance

- ◆ In 10 of 10 (100%) daratumumab-treated patient samples, results were consistent across all 3 independent runs
 - Results from all repetitions from a representative patient sample are shown in **Figure 6**
- ◆ There was 100% concordance between the evaluations of 2 independent reviewers
 - Reviewer evaluations were standardized using a brief form with set assessment criteria; those criteria and the reviewers' responses assessing the sample shown in **Figure 6** are tallied in **Table 1**

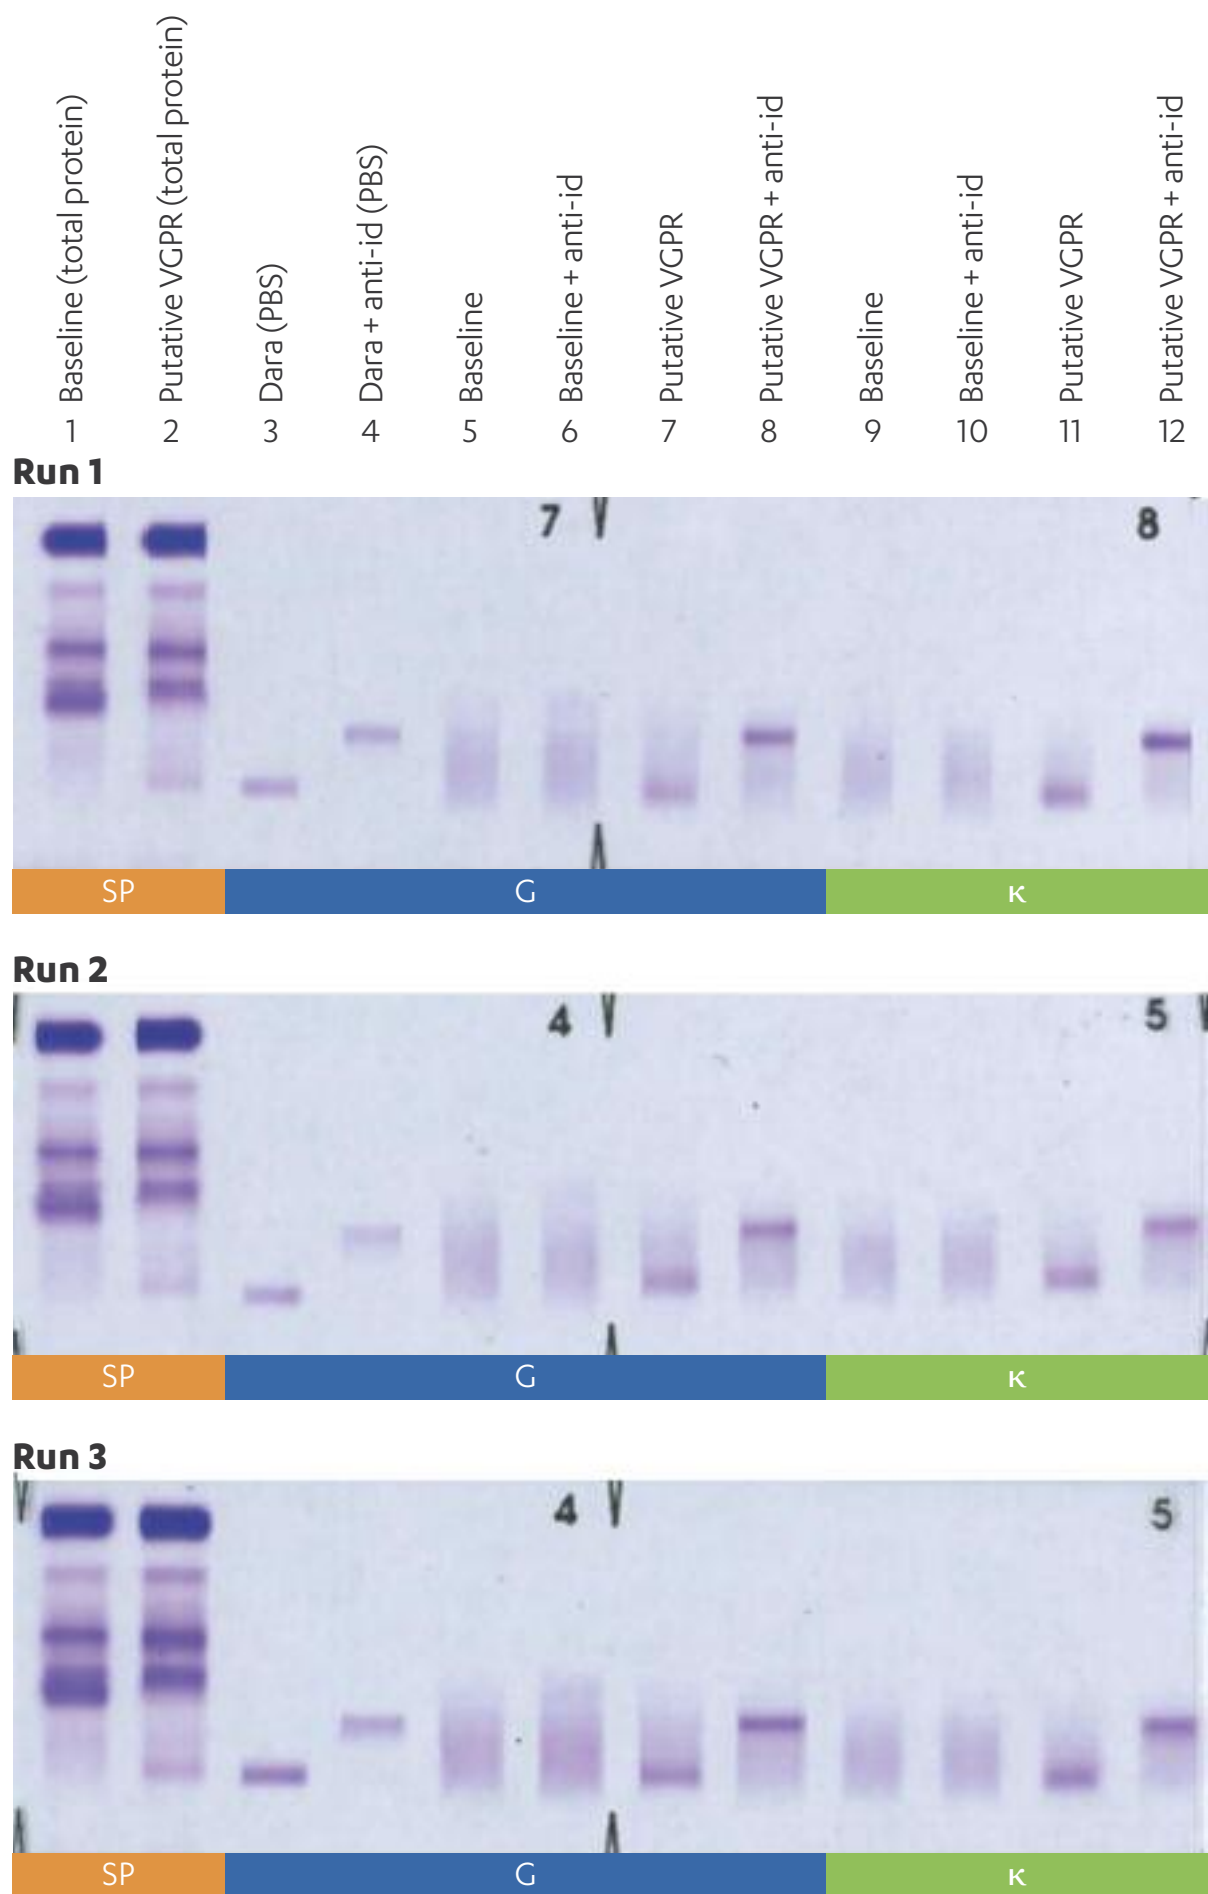

DIRA, daratumumab interference reflex assay; VGPR, very good partial response; Dara, daratumumab; PBS, phosphate-buffered saline; anti-id, anti-idiotypic; SP, total serum protein fix; G, IgG antisera; κ, kappa. Results for commercial sample 4 shown.

Figure 6. Reproducibility of DIRA results between independent experiments.

Identification of Clinical Responses

- ◆ DIRA differentiated daratumumab-treated patient samples containing residual M-protein (DIRA-positive) from those containing no M-protein (DIRA-negative)
- ◆ 33 samples from daratumumab-treated patients from a number of different studies were assessed for clinical response using DIRA
- ◆ 13 patients (39%) were DIRA-negative, 10 of whom were confirmed as having achieved CR based on bone marrow and FLC
- ◆ 20 (61%) were DIRA-positive and will continue to be monitored

ACKNOWLEDGMENTS

This study was supported by Janssen Research & Development, LLC. Editorial support was provided by Erica Chevalier-Larsen, PhD, of MedErgy, and was funded by Janssen Global Services, LLC.

Table 1. Concordance of Reviewer Assessments Between Experiments

Reviewer 1	Lane	Run 1	Run 2	Run 3
Migration of Dara + anti-id in control?	4 vs 3	Y	Y	Y
Migration of endogenous M-protein at baseline?	6 and 10	N	N	N
Migration of Dara in VGPR due to the disappearance of Dara (DD) or the appearance of Dara + anti-id complex (AC)?	8 vs 7 and 12 vs 11	Y DD + AC	Y DD + AC	Y DD + AC
Presence of M-protein after migration of Dara?	8 and 12	N	N	N
M-protein (M) or Dara (D)?		D	D	D
Conclusion		Negative	Negative	Negative
Reviewer 2	Lane	Run 1	Run 2	Run 3
Migration of Dara + anti-id in control?	4 vs 3	Y	Y	Y
Migration of endogenous M-protein at baseline?	6 and 10	N	N	N
Migration of Dara in VGPR due to the disappearance of Dara (DD) or the appearance of Dara + anti-id complex (AC)?	8 vs 7 and 12 vs 11	Y DD + AC	Y DD + AC	Y DD + AC
Presence of M-protein after migration of Dara?	8 and 12	N	N	N
M-protein (M) or Dara (D)?		D	D	D
Conclusion		Negative	Negative	Negative

Dara, daratumumab; anti-id, anti-idiotypic; Y, yes; N, no; VGPR, very good partial response.

CONCLUSIONS

- ◆ **DIRA is a specific, reproducible method to confirm the interference of daratumumab on serum IFE at 100 to 200 µg/mL**
- ◆ **DIRA-negative status warrants additional testing to confirm CR/sCR**
- ◆ **IMWG response criteria may require modification as mAbs receive approval for the treatment of MM**

REFERENCES

1. Zent CS, et al. *Blood*. 1998;91(9):3518-3523.
2. Rajkumar SV, et al. *Blood*. 2011;117(18):4691-4695.
3. McCudden CR, et al. *Clin Chem*. 2010;56(12):1897-1899.
4. Genzen JR, et al. *Br J Haematol*. 2011;155(1):123-125.
5. de Weers M, et al. *J Immunol*. 2011;186(3):1840-1848.
6. Lokhorst HM, et al. *J Clin Oncol*. 2014;32(15 suppl). Abstract 8513.
7. Plesner T, et al. *Blood*. 2014;124(21):84.
8. Axel AE, et al. Presented at: Annual Meeting of the American Association for Cancer Research; April 5-9, 2014; San Diego, CA. Abstract 2563.



An electronic version of the poster can be viewed by scanning the QR code. The QR code is intended to provide scientific information for individual reference. The PDF should not be altered or reproduced in any way.

Copies of this poster obtained through Quick Response (QR) Code are for personal use only and may not be reproduced without permission from ASCO® and the author of this poster.